Sterile bags

for microbiology

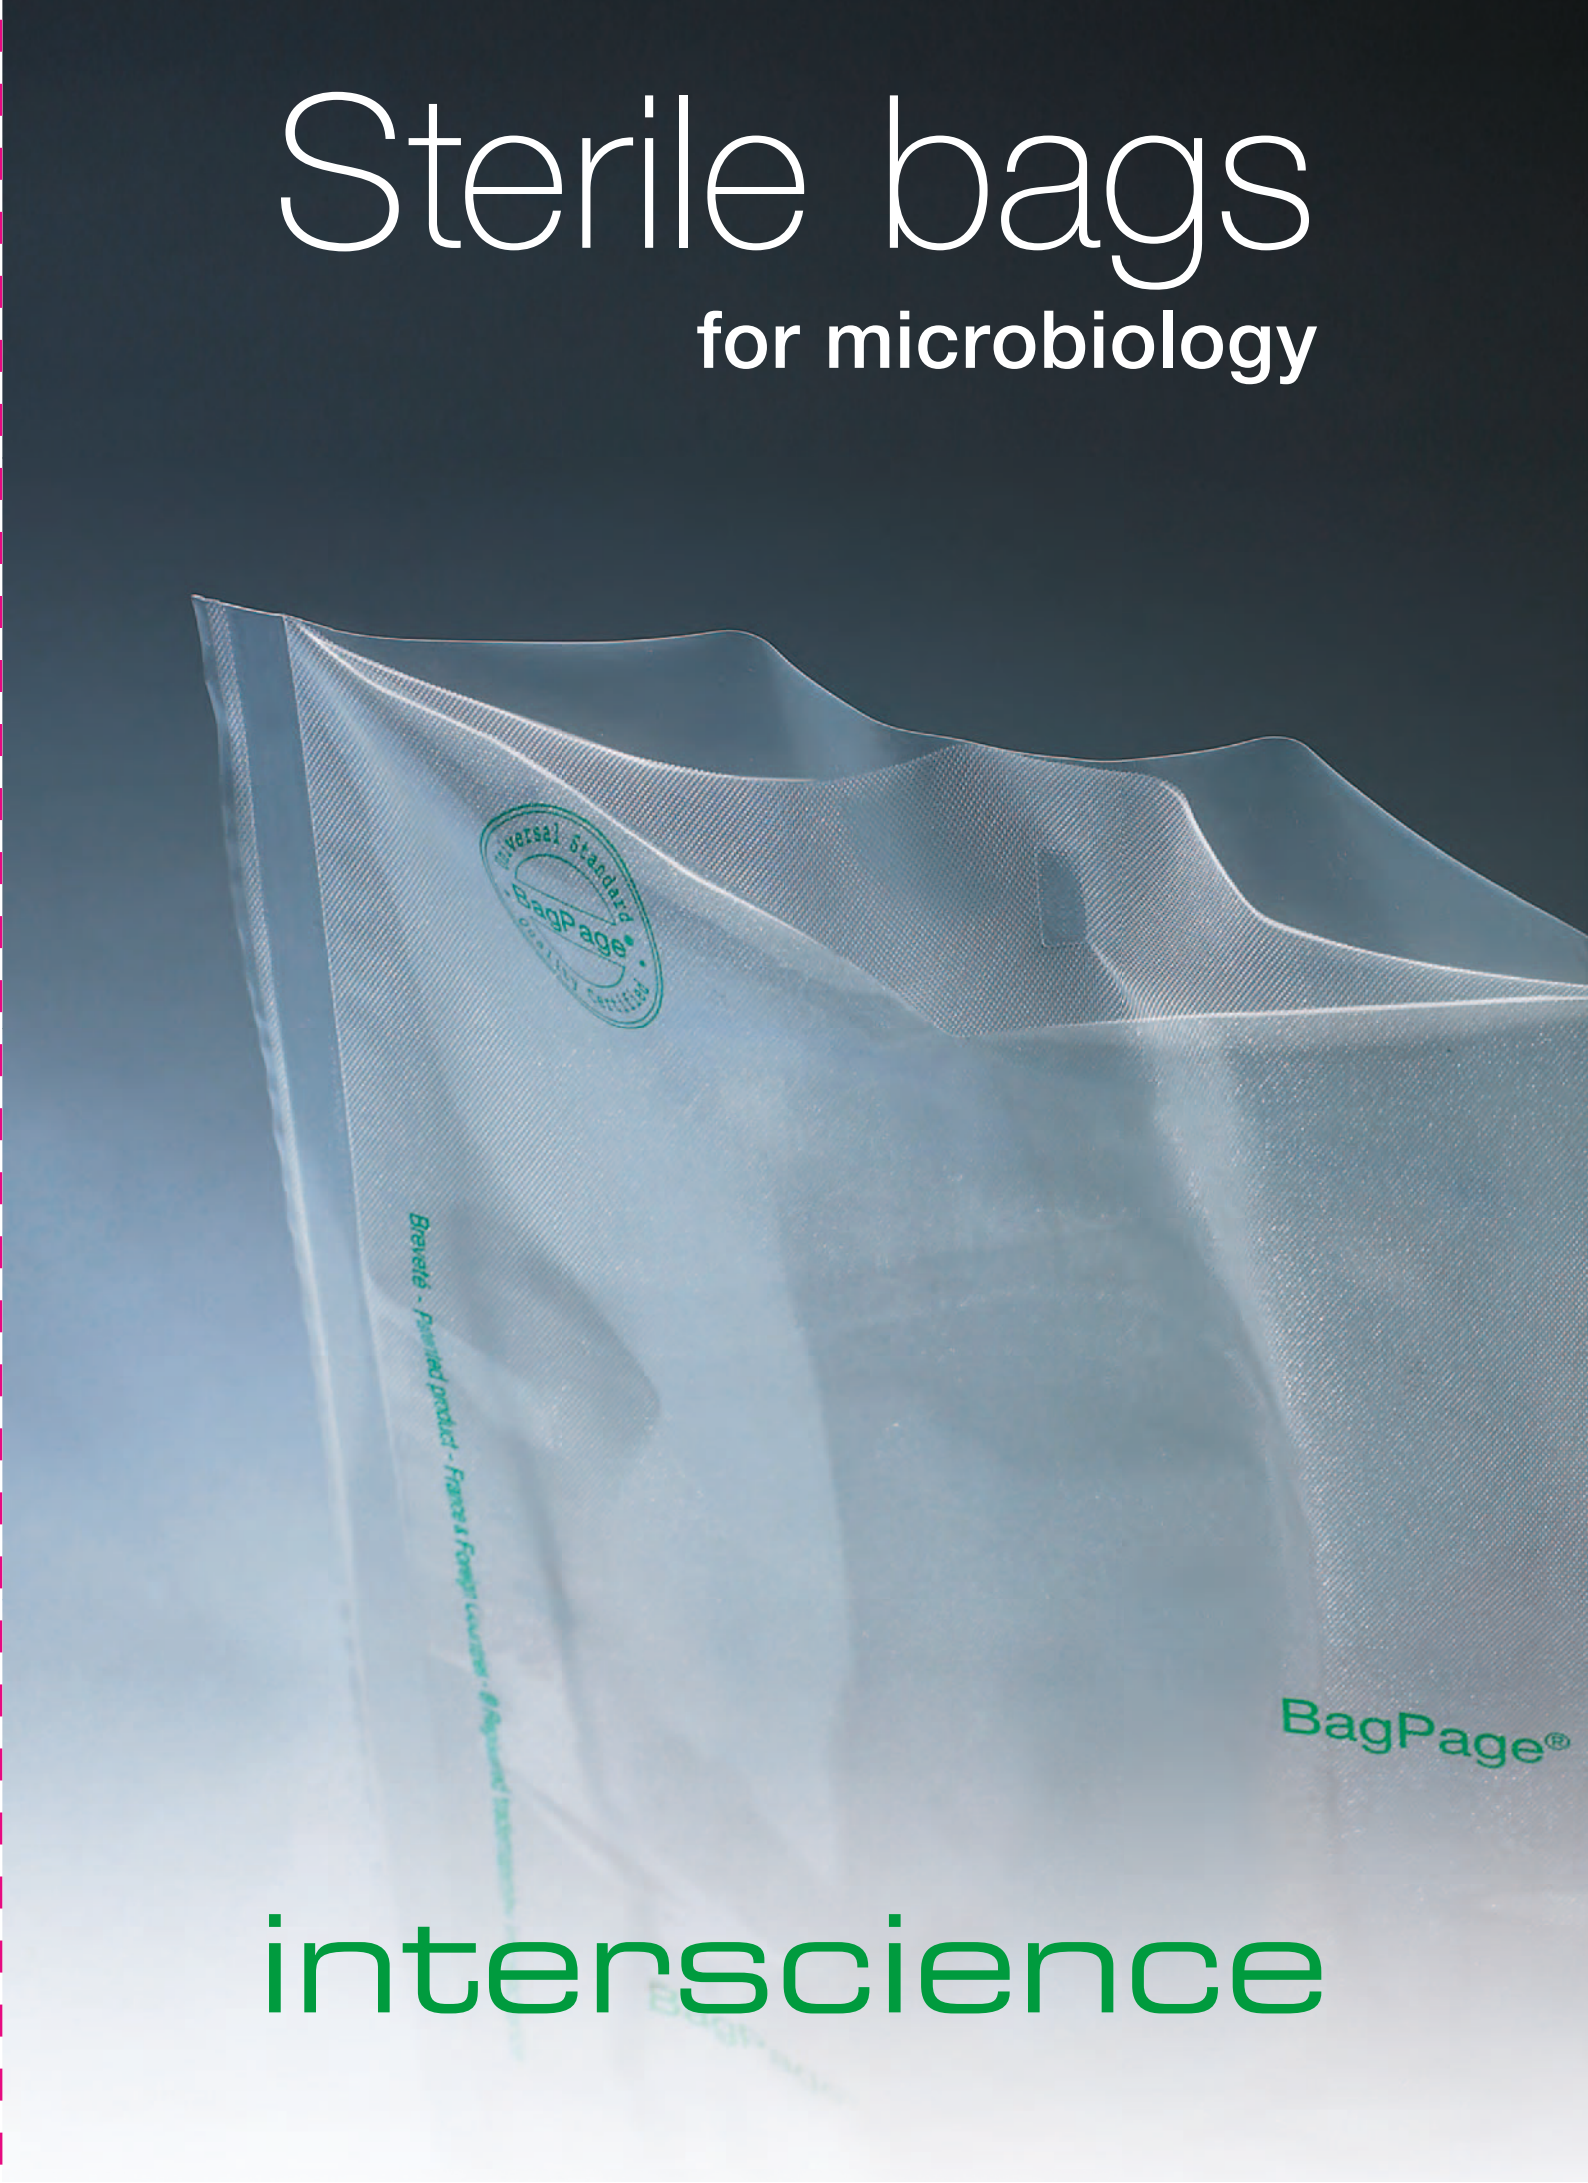

interscience

Choose your sterile blender bag

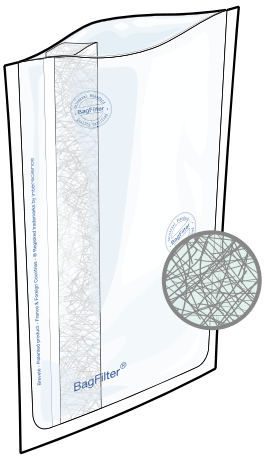

BagFilter® Side-filter ▸ For fibrous samples

- Non-woven side filter
- Multilayer®, reinforced multicoated complex
- Rigid and transparent

5 models, available in:
400 ml / 3500 ml

Filter porosity < 250 microns

BagFilter® P
non-woven filter

BagFilter® P
for pipetting



BagFilter® S
for pouring

BagFilter Pull-Up®
for small volumes / PCR

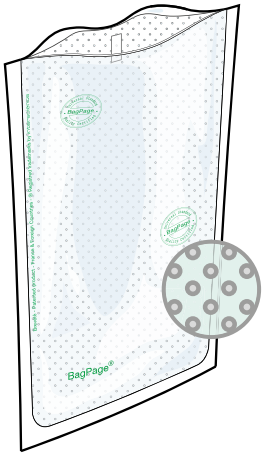

BagPage® Full-surface filter ▸ For pasty samples

- Full-surface micro-perforated filter
- Multilayer®, reinforced multicoated complex
- Rigid and transparent

9 models, available in:
80 ml / 100 ml / 400 ml / 3500 ml

Filter porosity: 280 microns

BagPage® +
micro-perforated filter

BagPage® F
for flow cytometry

BagPage® R
non-woven filter



BagPage® XR
extra resistant

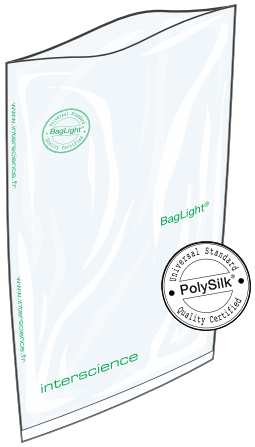

BagLight® Plain bag ▸ PolySilk® standard

- PolySilk®, polyolefin complex
- Flexible and transparent

6 models, available in:
100 ml / 400 ml / 3500 ml

Without filter

BagLight® PolySilk®
plain bag

BagLight® HD PolySilk®
easy labelling

BagLight® Multilayer®
ultra resistant

BagLight® Multilayer® U
round bottom

RollBag® Sampling and blender bag

- PolySilk®
- Individually sterile
- Writing zone

Model available in:
450 ml / 1300 ml

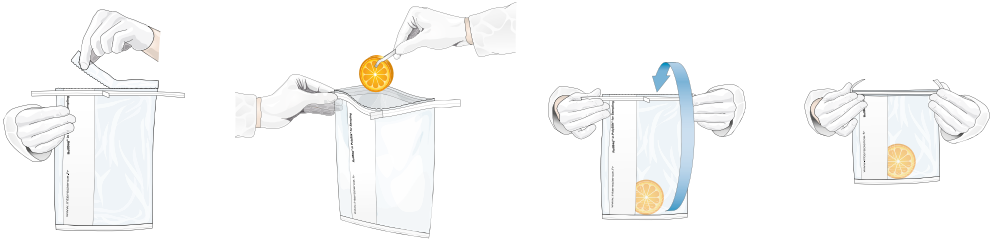

Technical specifications

Product	Ref.	Nom. vol.	Useful vol.	Filter porosity	Dimensions	Sterile pack of	Box of
BagFilter® Side-filter sterile blender bag for fibrous samples							
BagFilter® P 400	111 410	400 ml	50-300 ml	< 250 microns	190 x 300 mm	10	500
	111 425	400 ml	50-300 ml	< 250 microns	190 x 300 mm	25	500
BagFilter® P 400 unmarked	111 000	400 ml	50-300 ml	< 250 microns	190 x 300 mm	25	500
BagFilter® S 400	112 410	400 ml	50-300 ml	< 250 microns	190 x 300 mm	10	500
	112 425	400 ml	50-300 ml	< 250 microns	190 x 300 mm	25	500
BagFilter Pull-Up® (x25)	111 625	400 ml	50-300 ml	< 50 microns	190 x 300 mm	25	500
BagFilter® P 3500	113 510	3500 ml	200-2000 ml	< 250 microns	380 x 510 mm	10	100
BagPage® Full-surface filter sterile blender bag for pasty samples							
BagPage® 80	120 825	80 ml	5-40 ml	280 microns	160 x 95 mm	25	500
BagPage® 100	121 025	100 ml	5-50 ml	280 microns	180 x 95 mm	25	500
BagPage® + 400	122 010	400 ml	50-300 ml	280 microns	190 x 300 mm	10	500
	122 025	400 ml	50-300 ml	280 microns	190 x 300 mm	25	500
BagPage® + 400 unmarked	122 000	400 ml	50-300 ml	280 microns	190 x 300 mm	25	500
BagPage® F 400	122 325	400 ml	50-300 ml	63 microns	190 x 300 mm	25	500
BagPage® R 400	161 025	400 ml	50-300 ml	< 250 microns	190 x 300 mm	25	500
BagPage® U 400	122 225	400 ml	50-300 ml	280 microns	190 x 300 mm	25	500
BagPage® + XR 400	122 425	400 ml	50-300 ml	280 microns	190 x 300 mm	25	400
BagPage® + 3500	123 010	3500 ml	200-2000 ml	280 microns	380 x 510 mm	10	100
BagLight® Sterile plain blender bag / **PolySilk®**standard							
BagLight® 100 PolySilk®	131 025	100 ml	5-50 ml	-	110 x 185 mm	25	500
BagLight® 400 PolySilk®	132 025	400 ml	50-300 ml	-	175 x 300 mm	25	1000
BagLight® 400 HD PolySilk®	132 325	400 ml	50-300 ml	-	175 x 300 mm	25	1000
BagLight® 400 Multilayer®	132 225	400 ml	50-300 ml	-	190 x 300 mm	25	500
BagLight® 400 Multilayer® U	132 125	400 ml	50-300 ml	-	190 x 300 mm	25	500
BagLight® 3500 PolySilk®	133 025	3500 ml	200-2000 ml	-	380 x 510 mm	25	500
RollBag® Sterile sampling and blender bag							
RollBag® 450	145 010	450 ml	5-50 ml	-	110 x 230 mm	1000	1000
RollBag® 1300	145 040	1300 ml	50-300 ml	-	175 x 290 mm	500	500

Manufactured under ISO 9001-2000, all interscience **bags are food compatible, radio-sterilized and compatible with any blender. A sterilization red sticker is placed on every box. A sterilization certificate is included with each shipment.**

"A **good** analysis begins with a **good** bag"

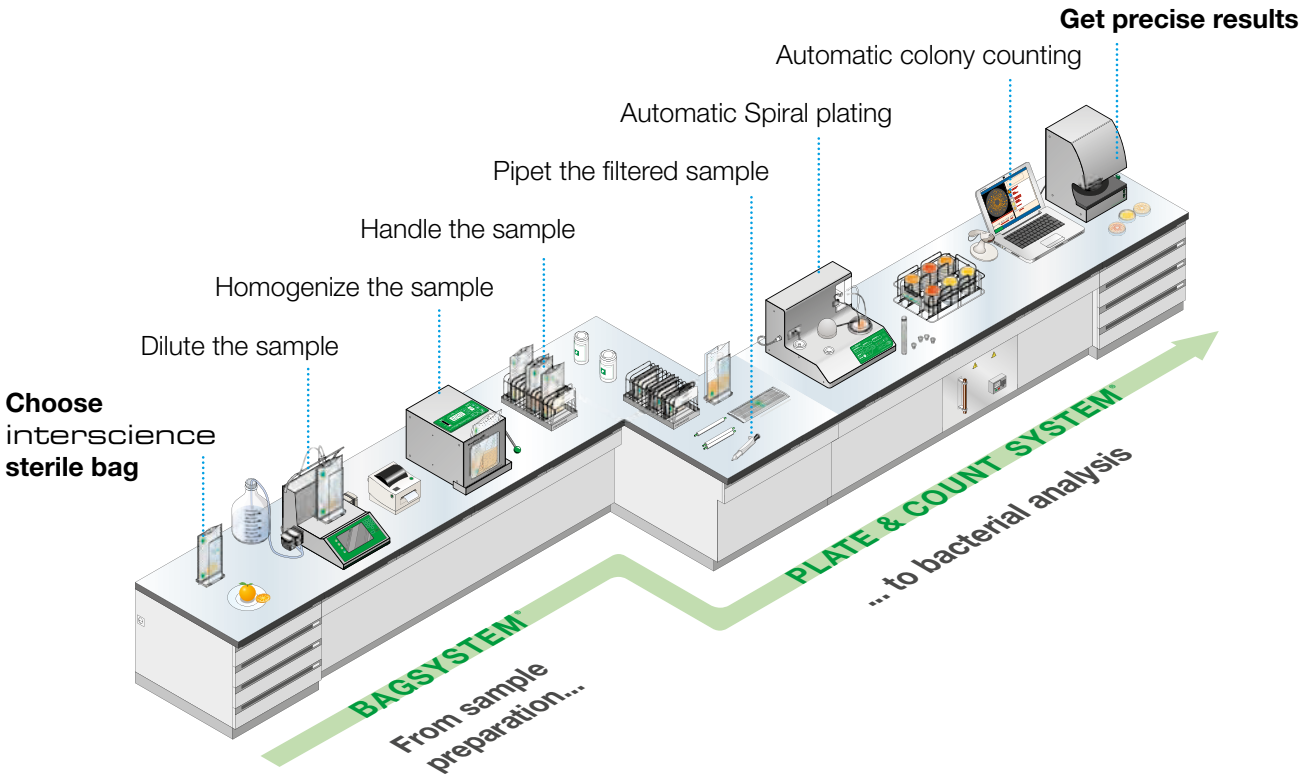

Choose **BagFilter®** for your sample preparation!

Here is a comparison of a sample* homogenized in a bag without a filter and in a **BagFilter®**. The bacterial concentration remains the same after filtration.

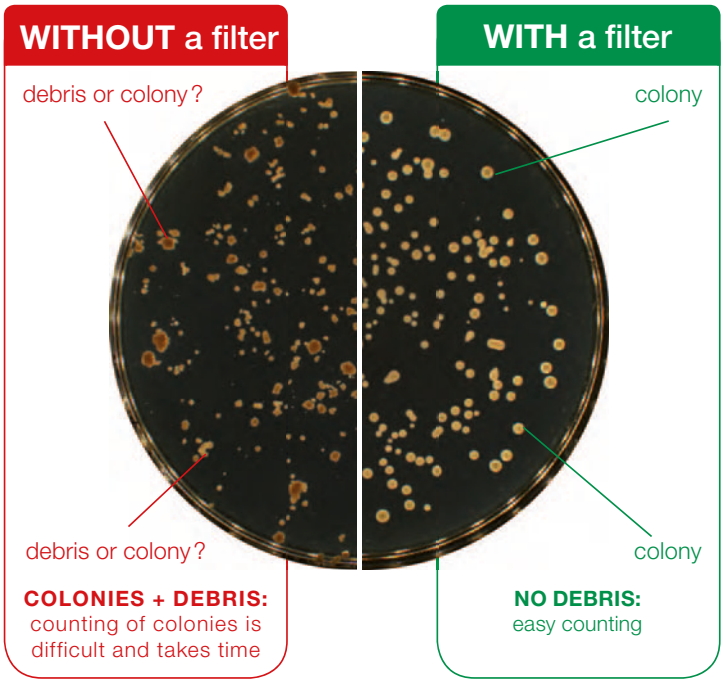

- **Time saver:**
  No sedimentation required
- **Colony counting optimized:**
  No debris on the Petri dish
- **Adapted to all samples:**
  More than 22 models of bags for every need

* Lactobacillus analysis in a cheese sample, plated on MRS agar incubated at 30°C for 48h.

HUBERLAB. AG
Industriestrasse 123
4147 Aesch

T 061 717 99 77
F 061 711 93 42

www.huberlab.ch
info@huberlab.ch

HUBERLAB.
committed to science