


Instructions for Use

CELLlevator™ - Stacking Device for CELLdisc™ (Item-No. 878071)

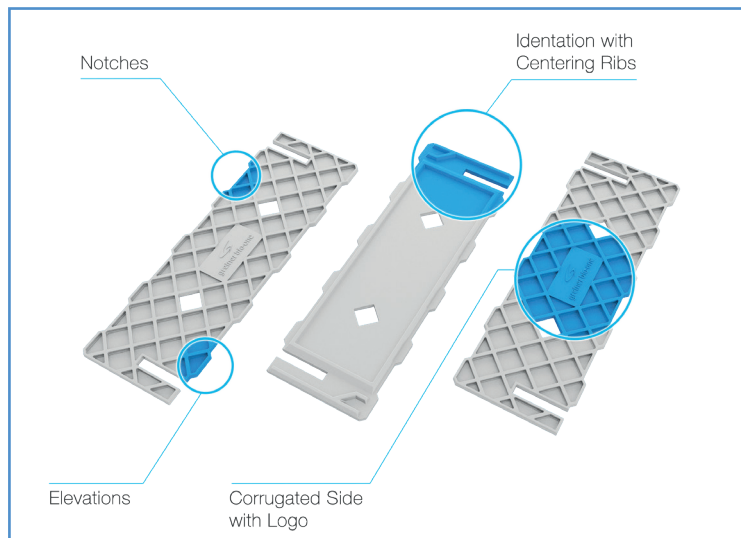

Intended Use

The CELLlevator™ facilitates easy and secure stacking of two CELLdisc™ devices.

Product Details

The CELLlevator™ consists of three identical segments with indentations and centering ribs which assembled form a triangle.

The corrugated side of the stripe with the Geiner Bio-One logo must always be on the outside of each part and the final stacking device.

→ Assembly guide on the reverse side →


Feature	Properties
Material	Polypropylene
Max. Loading Capacity	8 kg (refers to the assembled CELLlevator™)
Autoclavability	Yes (120 °C, 2 bar), max. 3 times*
TP-range	4°C-37°C
Sterility	No

* Autoclaving the CELLlevator™ more than 3 times is not recommended. After each autoclave cycle the integrity of the segments has to be analysed by the user.


HUBERLAB.

committed to science


CELLlevator™ - Assembling Guide

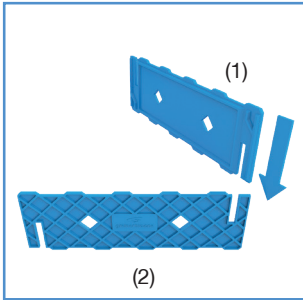


1 Join segment (1) with segment (2) using the indentations. Centering ribs at the side of the indentation guide the segments together.

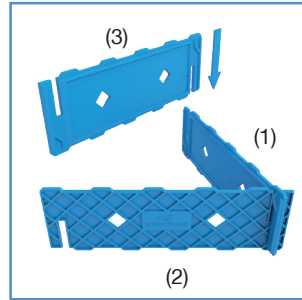


2 Join segment (3) accordingly with the indentation of segment (1) from above.

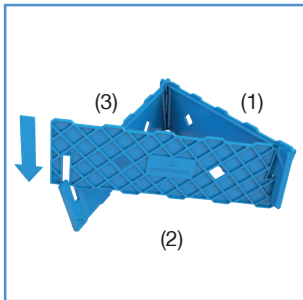


3 Lift segment (2) and insert into the remaining indentation from segment (3). Slight bending of the segments during the insertion is acceptable.

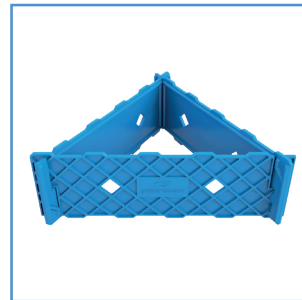

4 The final assembled CELLlevator™ should form a uniform triangle.

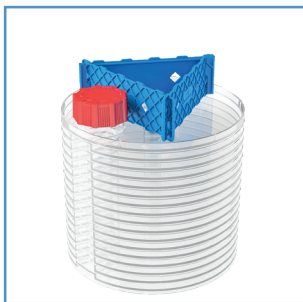

5 The CELLlevator™ must be positioned within the circumferential ring of the top plate of the CELLdisc™.

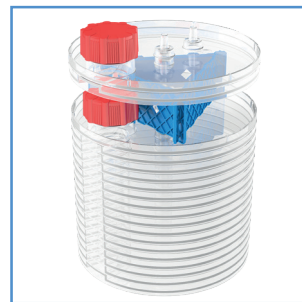

6 The other CELLdisc™ can now be positioned on top of the CELLlevator™. Ventilation of the lower CELLdisc™ is assured by the notches on the segments whereas planarity of the upper CELLdisc™ is assured by the elevations on the segments.